


Instruction and operation manual

PT100

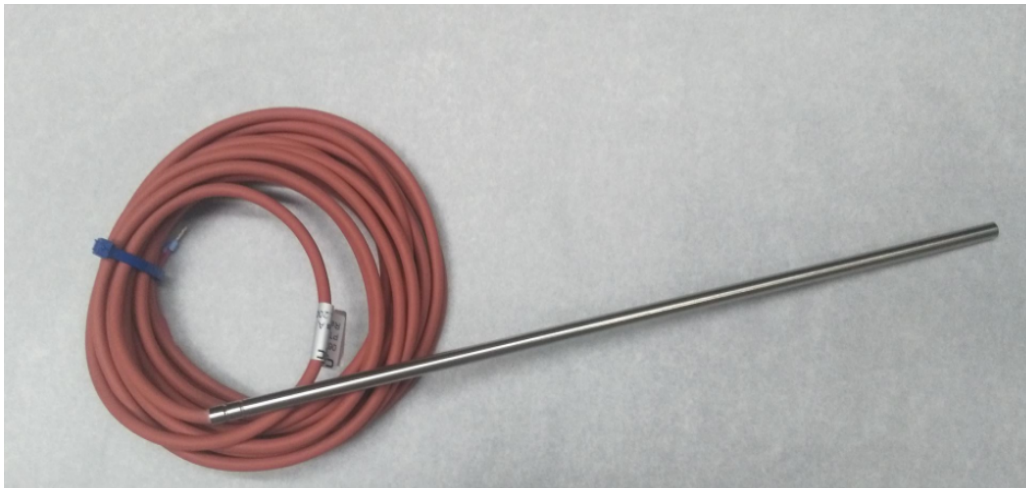

Revision: 2024-1-1
Modified: March, 2024

Dear Customer,

Thank you for choosing our product.

The operating instructions must be read in full and carefully observed before starting up the device. The manufacturer cannot be held liable for any damage which occurs as a result of non-observance or non-compliance with this manual.

Should the device be tampered with in any manner other than a procedure which is described and specified in the manual, the warranty is cancelled and the manufacturer is exempt from liability.


The device is destined exclusively for the described application.

SUTO offers no guarantee for the suitability for any other purpose. SUTO is also not liable for consequential damage resulting from the delivery, capability or use of this device.

Table of contents

1 Safety instructions.....	4
2 Registered trademarks.....	6
3 Application.....	7
4 Features.....	7
5 Technical data.....	8
5.1 General.....	8
5.2 Electrical data.....	8
5.3 Output-signals.....	8
5.4 Accuracy	8
6 Dimensional drawing.....	9
7 Determination of the installation point.....	9
8 Installation	10
8.1 Installation requirements.....	10
8.2 Installation procedure	10
8.3 Electrical connection	11
9 Optional extra accessories.....	11
9.1 Compression fitting	11
10 Calibration.....	11
11 Maintenance.....	11
12 Disposal or waste.....	12


1 Safety instructions



Please check if this instruction manual accords to the product type.

Please observe all notes and instructions indicated in this manual. It contains essential information which have to be observed before and during installation, operation and maintenance. Therefore this instruction manual has to be read carefully by the technician as well as by the responsible user / qualified personnel.

This instruction manual has to be available at the operation site of the PT100 at any time. In case of any obscurities or questions, regarding this manual or the product, please contact the manufacturer.




WARNING!

Compressed air!

Any contact with quickly escaping air or bursting parts of the compressed air system can lead to serious injuries or even death!

- Only use pressure tight installation material.
- Avoid that persons get hit escaping air or bursting parts of the instrument.
- The system must be pressureless during maintenance work.



WARNING!

Voltage used for supply!

Any contact with energized parts of the product, may lead to a electrical shock which can lead to serious injuries or even death!

- Consider all regulations for electrical installations.
- The system must be disconnected from any power supply during maintenance work.
- Any electrical work on the system is only allowed by authorized qualified personal.



ATTENTION!

Permitted operating parameters!

Observe the permitted operating parameters, any operation exceeding this parameters can lead to malfunctions and may lead to damage on the instrument or the system.

- Do not exceed the permitted operating parameters.
- Make sure the product is operated in its permitted limitations.
- Do not exceed or undercut the permitted storage and operation temperature and pressure.
- The product should be maintained and calibrated frequently, at least annually.

General safety instructions

- It is not allowed to use the product in explosive areas.
- Please observe the national regulations before/during installation and operation.

Remarks

- It is not allowed to disassemble the product.
- Always use spanner to mount the product properly.



ATTENTION!

Measurement values can be affected by malfunction!

The product must be installed properly and frequently maintained, otherwise it may lead to wrong measurement values, which can lead to wrong results.

- Do not exceed the maximum operation temperature at the sensors tip.
- Avoid condensation on the sensor element as this will affect the accuracy enormously.

Storage and transportation

- Make sure that the transportation temperature of the sensor is between -40 ... 100°C.

- For transportation it is recommended to use the packaging which comes with the sensor.
- Please make sure that the storage temperature of the sensor is between -40 ... 100°C.
- Avoid direct UV and solar radiation during storage.
- For the storage the humidity has to be <90%, no condensation.

2 Registered trademarks

SUTO®

Registered trademark of SUTO iTEC

MODBUS®

Registered trademark of the Modbus Organization, Hopkinton, USA

HART®

Registered trademark of the HART Communication Foundation, Austin, USA

PROFIBUS®

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany

3 Application

The PT100 is a sensor which is designed to measure the temperature of liquid, vapour, compressed air and gases within the permissible operating parameters. These parameters can be found in the technical data section.

The PT100 is not developed to be used in explosive areas. For the use in explosive areas please contact the manufacturer.

The PT100 is mainly used in compressed air systems in industrial environment.

4 Features

- Easy installation in compressed air systems.
- PT100 4-wire sensor.
- Measure the inlet / outlet temperature of dryers.
- Measure the outlet temperature of compressors
- IP67 casing provides robust protection in the industrial environment.

5 Technical data

5.1 General

CE	
Parameters	Standard unit temperature: °C
Principle of measurement	Resistance change
Sensor	PT100, class B
Measuring medium	Non-corrosive gases
Measuring range	-50 ... 180°C
Ambient temperature	-40 ... 85°C
Tube material	Stainless steel 1.4571
Cable	Silicon
Protection class	IP67
Dimensions	See dimensional drawing on page 9
Weight	0.175 kg

5.2 Electrical data

Power supply	8 ... 45 VDC / < 30 mA
--------------	------------------------


5.3 Output-signals

Analogue output	4 wire
-----------------	--------

5.4 Accuracy

Accuracy	0.5 % of reading + 0.2 % FS
----------	-----------------------------

6 Dimensional drawing

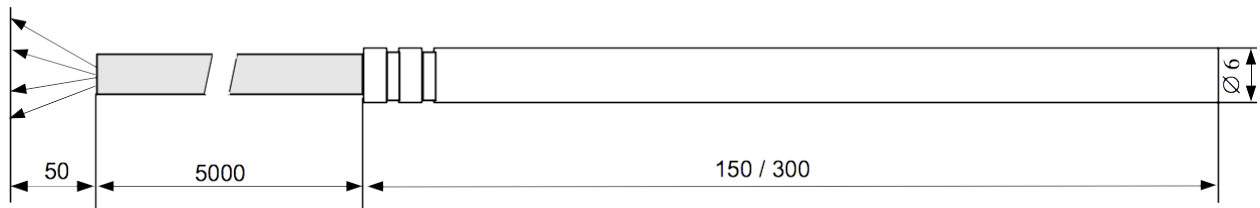

7 Determination of the installation point

In order to maintain the accuracy stated in the technical data, the sensor must be installed correctly. The sensor tip shouldn't contact the inner wall of the pipe, it will lead to wrong measurement values. For further instructions, please read the next chapter carefully.

Please consider that enough space exists at your site for a adequate installation as described in this manual.



ATTENTION!

Wrong measurement is possible, if the sensor is not installed correctly.

- Careful attention must be paid to the insertion depth of the sensor. Not less than 2/3 of the sensor shaft should be inside of the pipe.
- The sensor tip may not contact the inner wall of the pipe.
- The sensor is for indoor use only! At an outdoor installation, the sensor must be protected from solar radiation and rain.
- It is strongly recommend not to install the PT100 permanently in wet environment as it exists usually right after a compressor outlet.

8 Installation

Please make sure that all components listed below are included in your package.

Qty	Description	Item No.
1	PT100	S604 0102/ S604 0105
1	Instruction manual	No PN

8.1 Installation requirements

To install the PT100 a nozzle and a compression fitting is needed.

- The inner thread has to be G 1/2".
- The diameter of the hole must be ≥ 6 mm, other wise the shaft can not be inserted.

8.2 Installation procedure

The following steps explain the procedure of an appropriate installation.

Installation of the instrument


1. Screw the compression fitting tightly to the nozzle of the pipe.
2. Loosen the nut of the compression fitting.
3. Move the PT100 slightly through the compression fitting into the pipe.
 - Not less than 2/3 of the sensor shaft should be inside of the pipe.
 - The sensor tip may not contact the inner wall of the pipe.
4. Screw the nut of the compression fitting.

Removal of the instrument

1. Loosen the nut of the compression fitting.
2. Pull out the PT100 slowly.

8.3 Electrical connection

The PT100 is equipped with two white and two red cables. To connect the cables please have a look to the picture below.

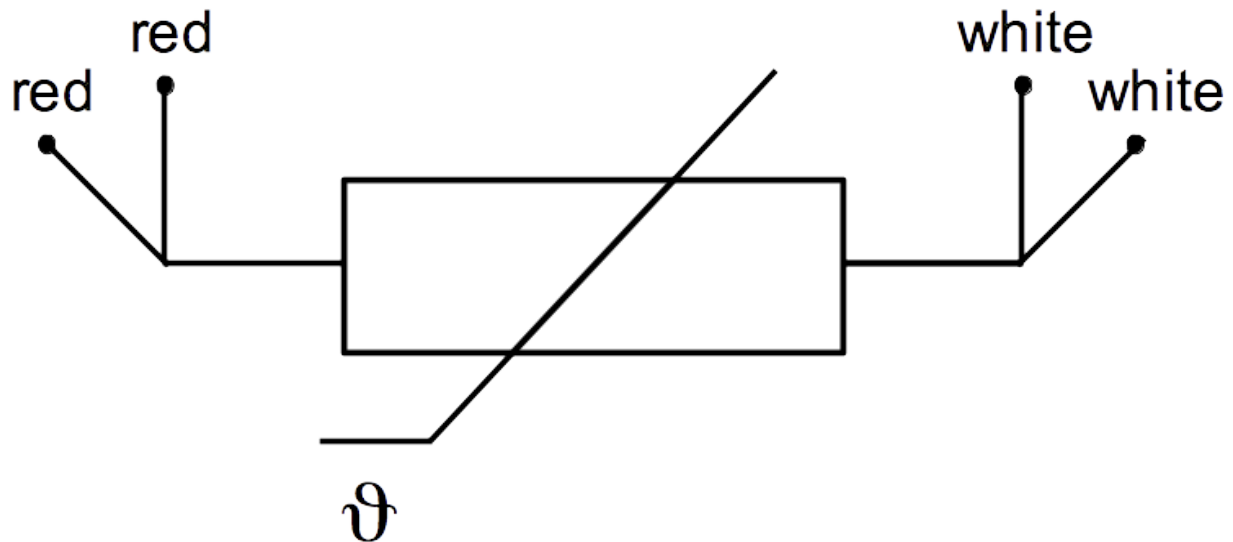

9 Optional extra accessories

9.1 Compression fitting

There are different types of compression fittings available:

- compression fitting 6mm, G1/2", PTFE ring, 0.6 MPa
- compression fitting 6mm, G1/2", metal ring, 1.6 MPa

10 Calibration

The sensor is calibrated ex work. The exact calibration date is printed on the certificate which is supplied together with the sensor. The accuracy of the sensor is regulated by the on site conditions, parameters like oil, high humidity or other impurities can affect the calibration and furthermore the accuracy. However we recommend to calibrate the instrument at least once per year. The calibration is excluded from the instruments warranty. For this please contact the manufacturer.

11 Maintenance

To clean the sensor and its accessories it is recommended to use moist cloth only.

12 Disposal or waste



Electronic devices are recyclable material and do not belong in the household waste.

The sensor, the accessories and its packings must be disposed according to your local statutory requirements.

The dispose can also be carried by the manufacturer of the product, for this please contact the manufacturer.

SUTO iTEC GmbH

Grißheimer Weg 21
D-79423 Heitersheim
Germany

Tel: +49 (0) 7634 50488 00

Email: sales@suto-itec.com

Website: www.suto-itec.com

All rights reserved ©

SUTO iTEC (ASIA) Co., Ltd.

Room 10, 6/F, Block B, Cambridge Plaza
188 San Wan Road, Sheung Shui, N.T.
Hong Kong

Tel: +852 2328 9782

Email: sales.asia@suto-itec.com

Website: www.suto-itec.com

Modifications and errors reserved

PT100_im_en_V2024-1-1
